



## HVPM-5

Pirani Vacuum transducer  
MEMS-Pirani and Piezo diaphragm sensor

QSG-HVPM-5-01, Revision: REVA, June 2020



### Quick start guide



### General information

Thank you for purchasing this Hositrاد product. This quick start guide contains important safety information and we encourage you to read this guide prior to installation and use of this product.

### Symbols used

Following symbols are used in the quick start guide:

**WARNING!** Critical information to prevent dangerous situations that can result in serious injury or death.

**CAUTION!** Important information to prevent dangerous situations that can damage the device or auxiliary equipment.

**ACTION!** Requires action or attention.

**INFORMATION:** Important recommendations and information for efficient use and best practice.

### Intended use

The HVPM-5 Pirani transducer is intended for vacuum gas pressure measurement and control within the limits listed in the specifications. The device is designed for screw in fittings mounting or KF fittings.

The device complies to EMC (Electro Magnetic Compatibility) class B immunity requirements for industrial environments.

### Safety information

This product should be installed and operated by technically skilled or trained personnel only.

**WARNING!** This product is not intended for installation and use in the presence of flammable gases or other explosive environments.

**WARNING!** Ensure that the gases exposed to the wetted materials are compatible with the wetted materials described in the specifications table and the used sealing materials.

**WARNING!** The pressure rating of the sensor element, connecting process fittings and sealing must comply with the maximum possible pressure in the application. The CE marking on the device does not apply to the pressure equipment directive.

**WARNING!** Ensure that the process connection is installed and tightened according to the recommended torque specification. Ensure that there are no leaks from the process connection when installing the transducer. Do not remove the transducer from the installation when the installation is either pressurized, evacuated, or contains hazardous fluids.

### Mechanical installation

The transducer is available with KF vacuum flange or screw-in fittings. When handling vacuum fittings always use gloves.

Refer to maximum allowed pressure, sealing method and assembly practices for the used fittings.

### KF fittings installation

1. Ensure that the centering O-ring and its sealing surfaces are clean and free of scratches or other damages.
2. Mount the supporting KF clamp.

### NPT flange installation

The NPT flange requires a suitable thread seal tape.

3. Screw the transmitter into the corresponding flange thread by hand.
4. Tighten it with a wrench using a torque of approx. 15 Nm.

**CAUTION!** Do not exceed tightening torque value.

Ensure that the process connection is leak tight using proper leak testing methods.

### Configuration and programming

The HVPM-5 can be user-configured, programmed and adjusted using the RS-232/RS-485 digital interface.

An optional USB programmer is available for programming the digital core of the transducer.

### Electrical installation


The HVPM-5 requires an external power supply supplying in the range 12-30 VDC. The external power supply shall be with safe isolation according to PELV (Protective Extra Low Voltage) requirements of EN60204-1.

The transducer is protected against momentary overvoltage on the supply line. The internal 100 mA thermal fuse will limit current draw in case of overvoltage to limit overheating. Additionally, the transmitter is protected against reverse polarity caused by incorrect wiring to the power supply.

The transducer electronics have a high level of immunity against external electromagnetic interference. Braided shielded cables are required to comply with the immunity requirements according to EN61326-1 for industrial locations.

### Electrical connection (9 pin D-sub and 15 pin D-sub)

The transducer provides a voltage signal proportional to the measured pressure.

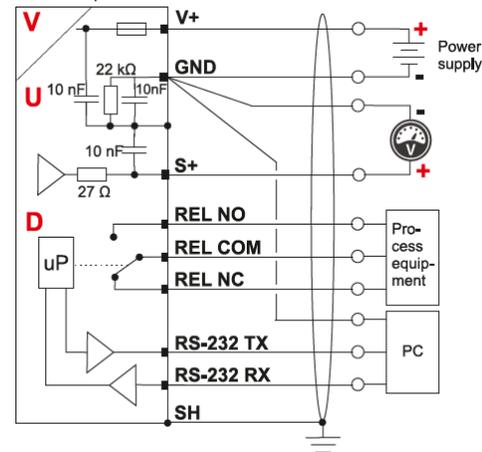


**INFORMATION:** It is recommended to use a differential input to measure the output signal that uses a separate signal return wire connected to the transmitter connector. If power supply return and signal return share the same wire connection the voltage drop as function of supply current will cause a measurement deviation. In that case, the measurement deviation will increase with the cable length.

### Connector pinout and cable wiring

#### 15 Pin HD D-sub RS-232 / RS-485

Pin	Description
1	RS-232 Transmit / RS-485 (-)
2	RS-232 Receive / RS-485 (+)
3	Supply voltage + (12-30 VDC)
4	Supply voltage - (return)
5	Analog voltage signal +
6	Analog voltage signal - (return)
7	Relay 1 NO <sup>(1)</sup>
8	Relay 1 Common <sup>(2)</sup>
9	Relay 1 NC <sup>(3)</sup>
10	Relay 2 NC <sup>(3)</sup>
11	Relay 2 Common <sup>(2)</sup>
12	Relay 2 NO <sup>(1)</sup>
13	Relay 3 NC <sup>(3)</sup>
14	Relay 3 Common <sup>(2)</sup>
15	Relay 3 NO <sup>(1)</sup>




- (1) Optional relay - normally open contact
- (2) Optional relay - common contact
- (3) Optional relay - normally closed contact

The solid-state relay is a hardware option that needs to be specified when ordering the part. The setpoint value can be programmed using the H-Connect™ or RS-232/RS-485 digital interface. For programming of setpoint values refer to the full operating instructions.

#### 9 Pin D-sub RS-232 / RS-485

Pin	Description
1	Relay NO <sup>(4)</sup>
2	Relay NC <sup>(5)</sup>
3	Supply voltage + (12-30 VDC)
4	Supply voltage - (return)
5	Analog voltage signal +
6	Relay Common <sup>(6)</sup>
7	RS-232 Transmit / RS-485 (-)
8	Analog voltage signal - (return)
9	RS-232 Receive / RS-485 (+)




- (4) Optional relay - normally open contact
- (5) Optional relay - normally closed contact
- (6) Optional relay - common contact

The solid-state relay is a hardware option that needs to be specified when ordering the part. The setpoint value can be programmed using the RS-232/RS-485 digital interface. For programming of setpoint values refer to the full operating instructions.


#### 6 Pin Hirschmann connector

Pin	Description
1	Identification resistor (3K)
2	Analog voltage signal +
3	Analog voltage signal - (return)
4	Supply voltage 12-30 VDC
5	Supply voltage - (return)
6	Chassis



## 8 pin RJ45 / 8P8C

Pin	Description
1	Supply voltage 12-30 VDC
2	Supply voltage – (return)
3	Analog pressure voltage signal +
4	Identification resistor <sup>(7)</sup>
5	Analog voltage signal – (return)
6	Relay 2 NO <sup>(8)</sup>
7	Relay 1 NO <sup>(8)</sup>
8	Relay 1 & 2 Common <sup>(9)</sup>




- (7) For ID resistor values refer to installation and operating manual.  
 (8) Optional relay - normally open contact.  
 (9) Optional relay – common contact.  
 The solid-state relay is a hardware option that needs to be specified when ordering the part. For programming of setpoint values refer to Operation & Installation manual.

## Signal to pressure conversion (0-10 VDC voltage output)

The transducer can provide a voltage output from 0-10 VDC and is available with different pre-configured output scaling.

When the transducer is configured for 1 VDC/decade output, the voltage signal ( $u$ ) can be converted to pressure using the following linear expression:

$$\text{Voltage to pressure conversion: } P(u) = 10^{(u-6.5)}$$

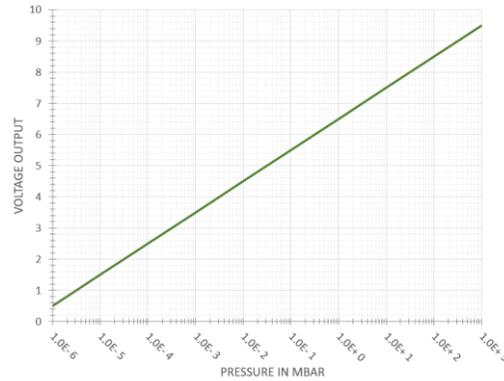

**INFORMATION:** Refer to Operation & Installation manual for conversion and scaling of other analog outputs. The transducer may be configured with other analog scaling than the standard 1 VDC/decade output.

## Measurement

The HVPM-5 Pirani is intended for measurement in the range 1.0E-6 to 1,333 mbar.

When used in the range below 1.0E-5 mbar it is required to ensure adequate outgassing of water vapor from the internal surfaces of the transducer. After installing the transducer, it is recommended to perform a zero adjust either by pressing the zero switch or sending the digital zero command when a base pressure below 5.0E-7 mbar is achieved. Before performing any adjustment or calibration refer to procedure described in the Operation & Installation manual.

## Status LED

The LED indicator signals the transducer status and can indicate following basic indications:

### Startup sequence

- 0.5 s purple followed by 4 s green pulse

### Normal standard operation

- Solid green

### Sensor fail stage

- 1 s flash cycle

Refer to Operation & Installation manual for complete LED status indications.

## Maintenance

Maintenance is not required during the lifecycle of this product. Depending on the application, the calibration may shift during the life-time and re-calibration can be performed by the user. Refer to HVPM-5 the Operation & Installation manual. The HVPM-5 can be user configured, calibrated and tested using the digital interface.

## Return

Proper return forms and a return materials authorization (RMA) must be filled out before returning a product to Hositrad. The RMA procedure can be found on:

## Disposal in the European Union

At the end of life of this product, it must be disposed according to the European Directive 2012/19/EU (WEEE). This product should not be mixed with general household waste.



**WARNING!** If the product has been exposed to human or environmental hazards materials during its use, ensure proper decontamination before disposal.

For proper treatment, recovery and recycling, please take this product to designated collection points. Please contact your local authority for further details of your nearest designated collection point.

For questions regarding disposal please contact your dealer or Hositrad for further information.

## Specifications

Specifications	
Measuring range in mbar	1×10 <sup>-6</sup> to 1,333 mbar (7.5×10 <sup>-7</sup> to 1000 Torr)
Measuring principle 1×10 <sup>-6</sup> to 1.5 mbar	MEMS Pirani thermal conductivity
Measuring principle 1.5 to 2 mbar	Blended MEMS Pirani / piezo reading
Measuring principle 2 to 1,333 mbar	MEMS piezo resistive diaphragm
Accuracy <sup>(10)</sup> 1×10 <sup>-5</sup> to 9.99×10 <sup>-5</sup>	25% of reading
Accuracy <sup>(10)</sup> 1×10 <sup>-4</sup> to 9.99 mbar	5% of reading
Accuracy <sup>(10)</sup> 10.00 to 99.9 mbar	1% of reading
Accuracy <sup>(10)</sup> 100 to 800 mbar	0.5% of reading
Accuracy <sup>(10)</sup> 800 to 1099 mbar	0.25% of reading
Accuracy <sup>(10)</sup> 1100 to 1200 mbar	0.5% of reading
Hysteresis 1×10 <sup>-3</sup> to 10 mbar	1% of reading
Hysteresis 10 to 1,333	0.1% of reading
Vacuum temperature sensor range	-20 to +85 °C
Analog output resolution	16 bit (150 µV)
Analog output update rate	124 Hz
Response time (ISO 19685:2017)	<20 ms
Temperature compensation	+10 to +50 °C
Solid state relay set point range	5×10 <sup>6</sup> to 1200 mbar (3.75×10 <sup>6</sup> to 900 Torr)
Solid state relay contact rating	50 V, 100 mA <sub>rms</sub> / mA <sub>dc</sub>
Solid state relay approvals	UL Recognized: File E76270, CSA Certified: Cert. 1175739, EN/IEC 60950-1 Certified
Environment conditions	
Operating ambient temperature	-20 to +50 °C
Media temperature	-20 to +50 °C
Storage ambient temperature	-40 to +120 °C
Bake-out temperature (non-operating)	+120 °C
Maximum media pressure	10 bar absolute <sup>(11)</sup>
Mounting position	Arbitrary
Protection rating, EN 60529/A2:2013	IP40
Humidity, IEC 68-2-38	98%, non-condensing


- (10) Accuracy specifications are typical values measured with Nitrogen gas at stable temperature after zero adjustment.  
 (11) Overpressure limits only applicable with using fittings rated to the specified maximum pressure.

## Specifications (continued)

Materials	
Enclosure	AISI 304L Stainless Steel / Aluminum 6061
Vacuum flange (media wetted)	AISI 304L Stainless Steel
Vacuum exposed materials (media wetted)	AISI 304L Stainless steel, Kovar, glass, silicon, nickel, aluminum, SiO <sub>2</sub> , Si <sub>3</sub> N <sub>4</sub> , gold, Viton®, low out-gassing epoxy resin, solder and RO4350
Process leak tightness	<1·10 <sup>-9</sup> mbar-l/sec.
CE	Directive 2014/30/EU
RoHS compliance	Directive EU 2015/863
Power supply	
Supply voltage	12-30 VDC
Power consumption	240 mW (max)
Reverse polarity protection	Yes
Overvoltage protection	Yes
Internal fuse	100 mA (thermal recoverable)

Specifications are subject to change without further notice  
 Viton® is a trademark of THE CHEMOURS COMPANY FC, LLC

## Dimensions



All dimensions are in mm unless otherwise stated – General tolerance ISO 2768-1 M

For dimensions of other flange types refer to Operation & Installation manual.

## Declaration of Conformity

This declaration of conformity has been made in accordance with EN ISO/IEC 17050-1:2010

Manufacturer:	Hositrad B.V.
Address:	De Wel 44 3871 MV Hoevelaken Holland

We hereby declare under our sole responsibility that the following products:

Product description:	Vacuum Transmitter
Product part number	HVPM-5-xxxxxxx

Complies with the requirements of following relevant European Union harmonization directive:

Electromagnetic Compatibility (EMC) Directive 2014/30/EU
RoHS Directive EU 2015/863

Conformity is assessed in accordance to the following standards:

Reference: Date	Title
EN61326-1: 2013	Product family standard, Measurement, control and laboratory equipment
EN50581: 2012	Technical documentation for the assessment of electrical and electronic products with respect to the restriction of hazardous substances

Signed on behalf of:	Hositrad B.V.
Place of issue:	3871 MV Hoevelaken, Holland
Date of issue:	June 23 <sup>rd</sup> 2020
Signature:	

Name, Title: Jurgen Tomassen, Chief Executive Officer

This declaration of conformity is available online at: [www.Hositrad.com/doc.htm](http://www.Hositrad.com/doc.htm)

Document number: DOC-HVPM-5-01, Revision: A



## Warranty and disclaimer

Hositrad warrants this product to be free from defects in materials and workmanship for a period of 24 months from the date of the delivery.

Warranty does not cover:

- Mechanical or corrosive damage to the sensor diaphragm
- Physical or deposition contamination of the sensor diaphragm
- Damage caused by shipping
- Normal wear and tear
- Incorrect use or installation
- Operation beyond the published design limits

Hositrad is not liable for any claims arising from improper use, incorrect installation or use with gases or liquids not compatible with the media wetted materials described in the specifications table. Hositrad is not liable for loss of profits or revenue, overheads, loss of data, reinstallation costs, damage to other equipment or any incidental or consequential damages of any nature.

